
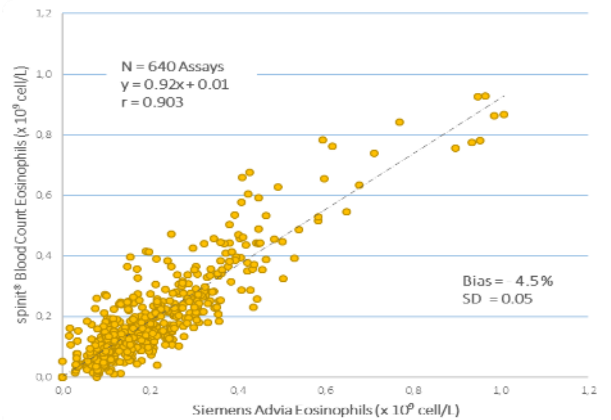
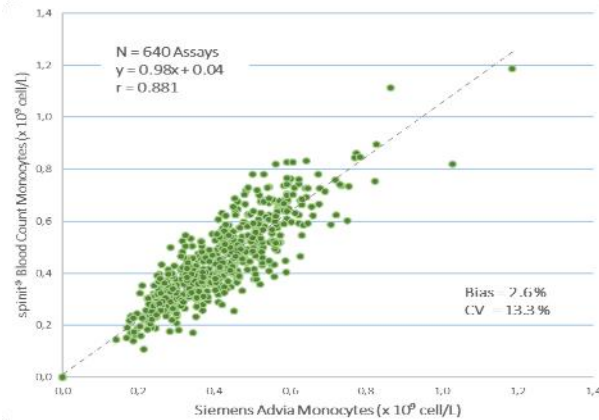
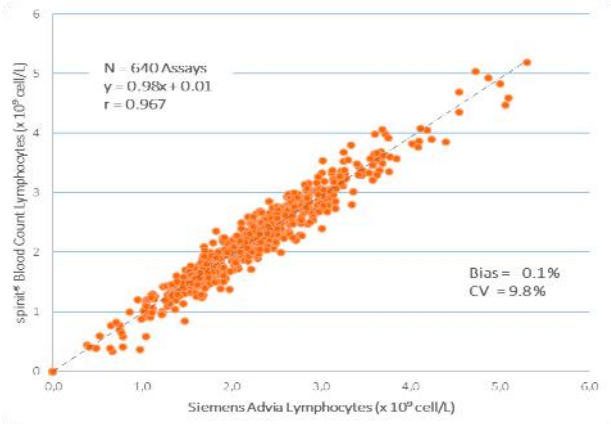
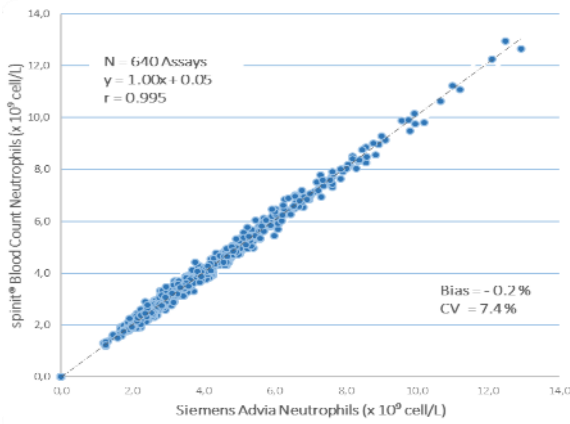
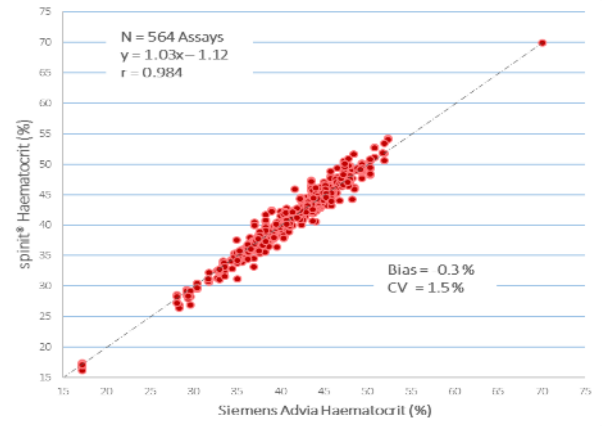


Key Features

- One small drop of blood - 15 µL
- Short assay time
- Simplicity
- Advanced fail-safe mechanisms

Method Comparison

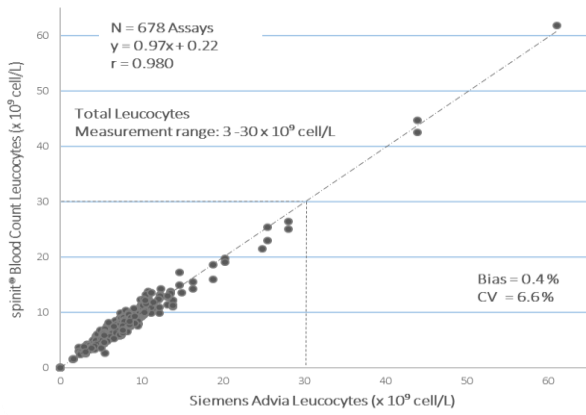

Method Comparison studies performed by using 8 different spinit[®] instruments and 14 cartridge lots. All whole blood samples were analysed in duplicate. Reference method = Siemens ADVIA. Studies performed according to CLSI guideline EP5-A2, EP6, EP7-A2, EP9-A2 and methods detailed in Clin. Chem. 21(13) 1935 (1975).

Contacts

Designed, developed & manufactured by biosurfit SA
 Rua 25 de Abril n°66 | 2050-317 Azambuja, Portugal
 Email: info@biosurfit.com

Following ISO13485
 Certified by TÜV Rheinland
 www.biosurfit.com

